

FIG. 1
PRIOR ART

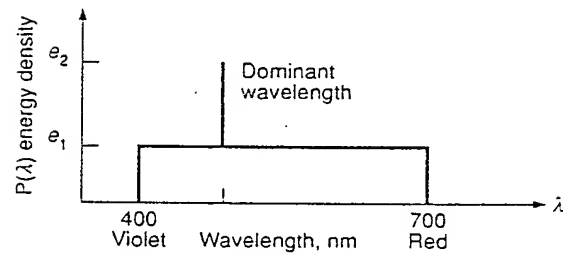


FIG. 2
PRIOR ART

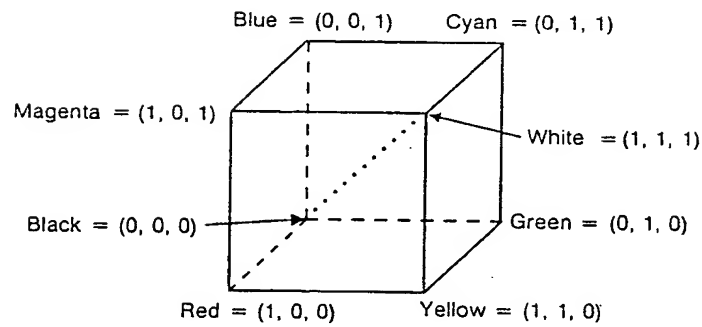


FIG. 3
PRIOR ART

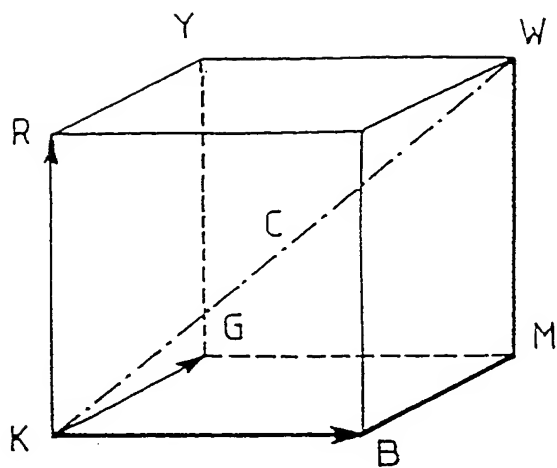


FIG.4A
PRIOR ART

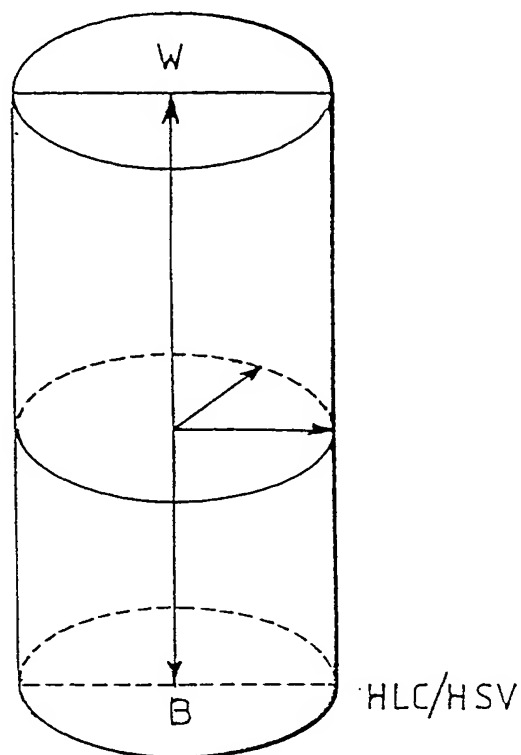


FIG.4B
PRIOR ART

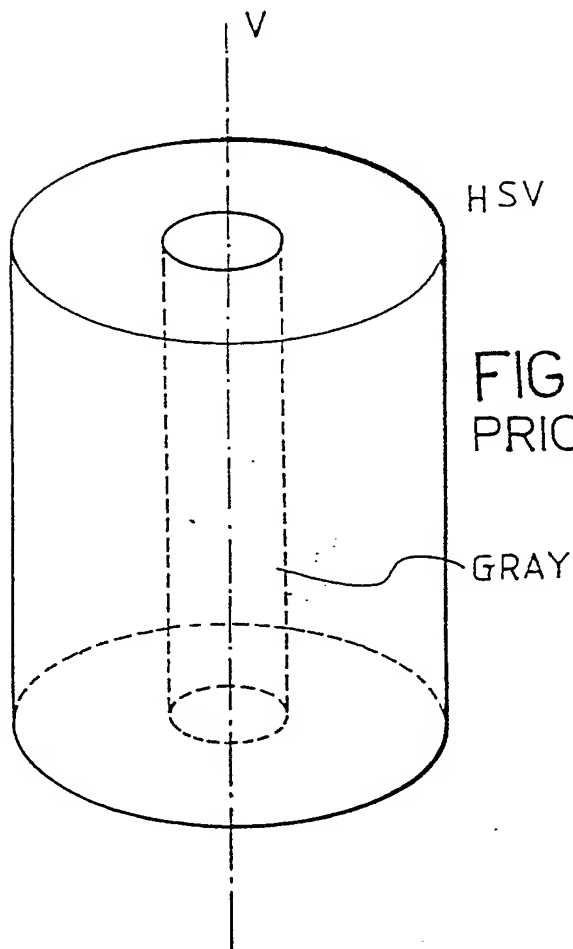


FIG.5
PRIOR ART


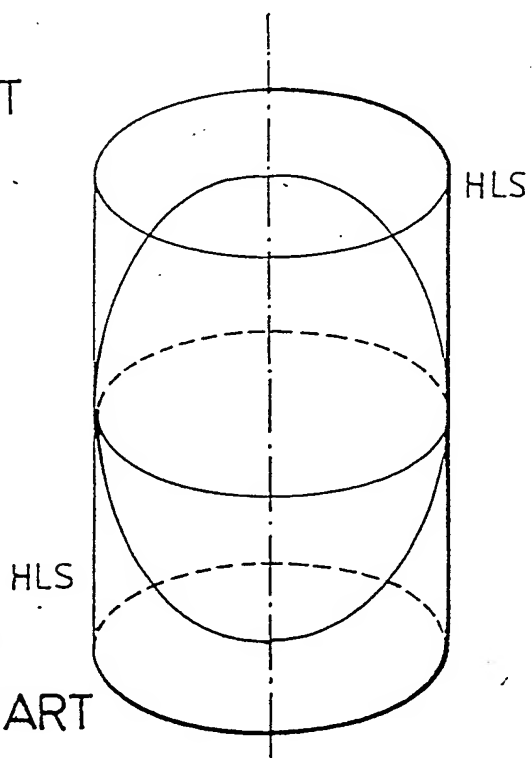



FIG.6
PRIOR ART

3/12

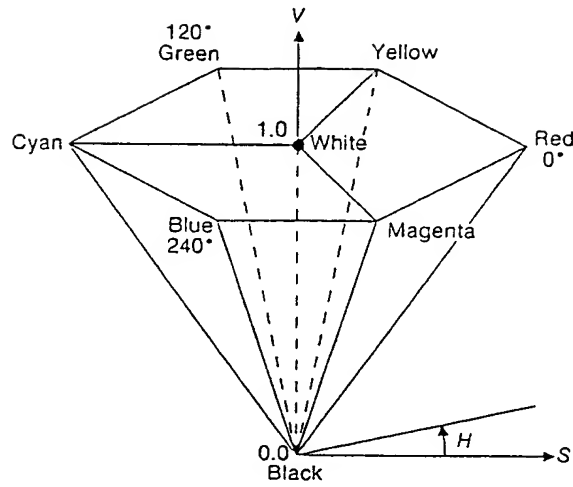


HSV

FIG. 7
PRIOR ART

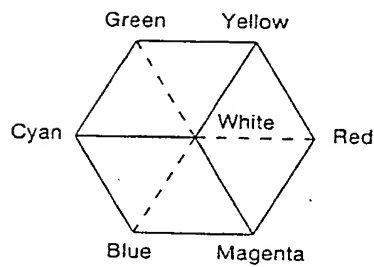



HSV Projection




FIG. 8
PRIOR ART

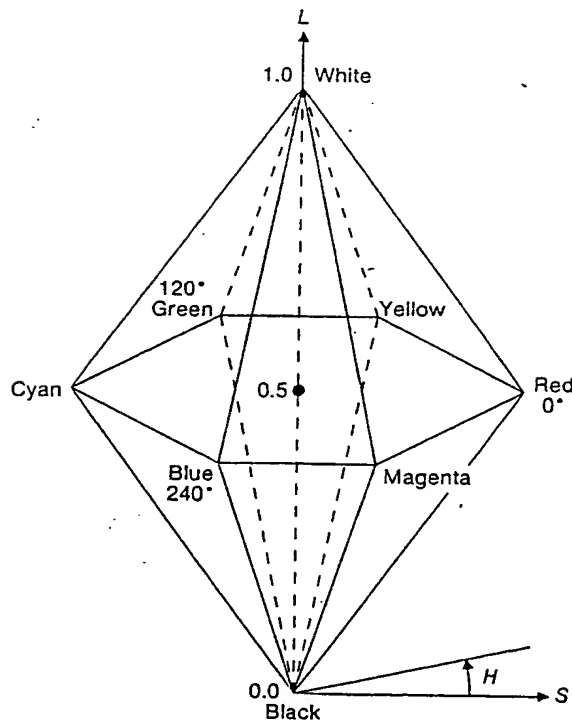

HLS

FIG. 9
PRIOR ART

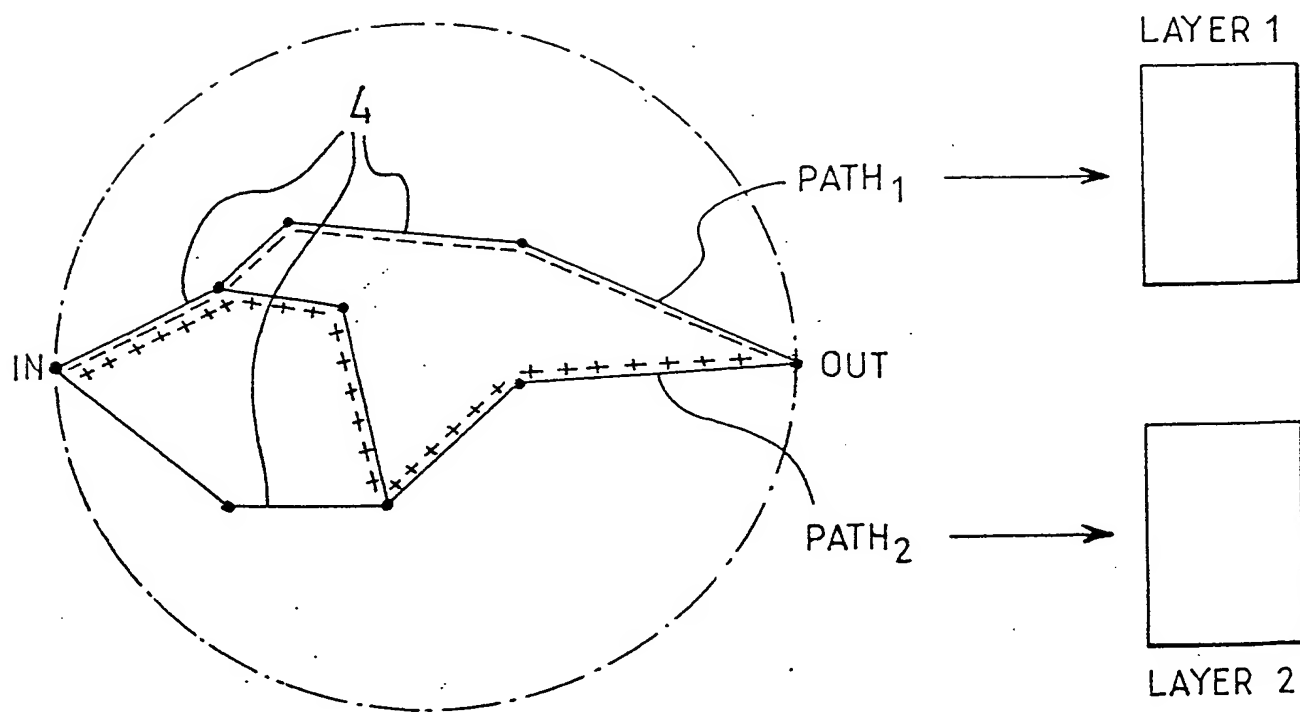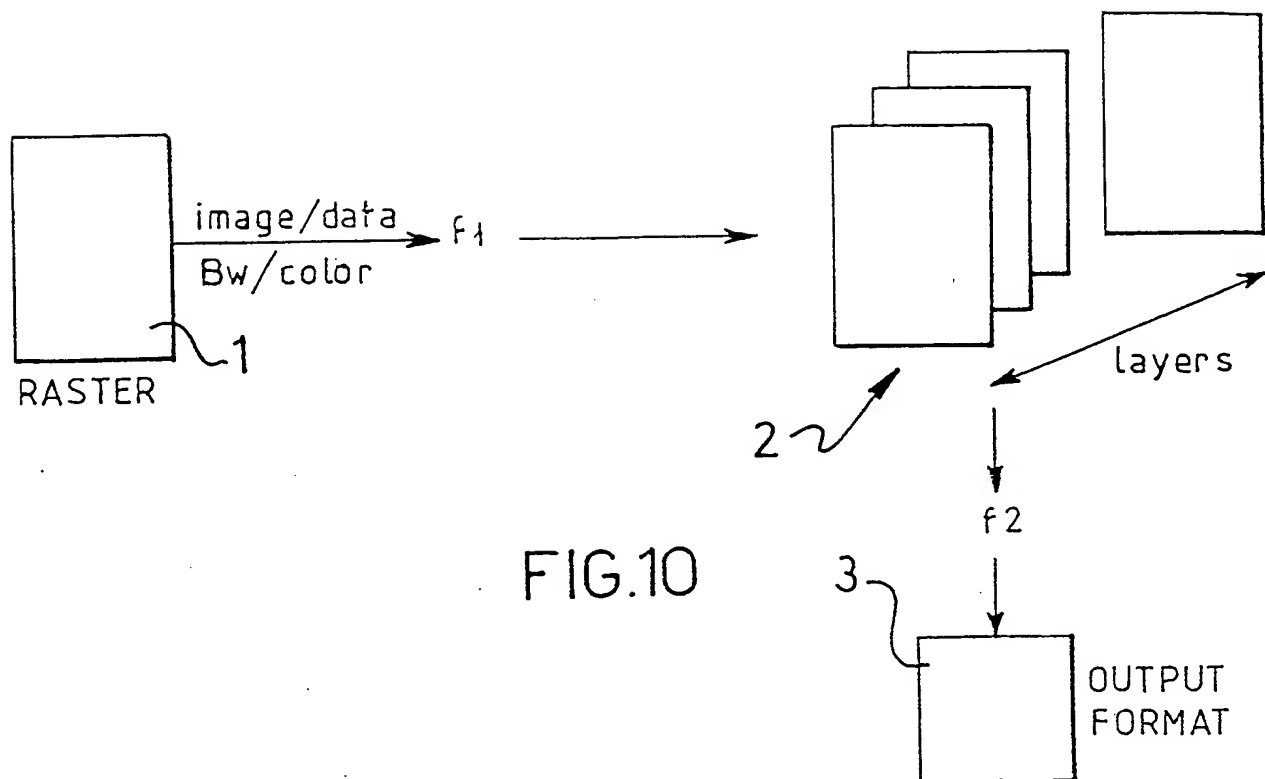

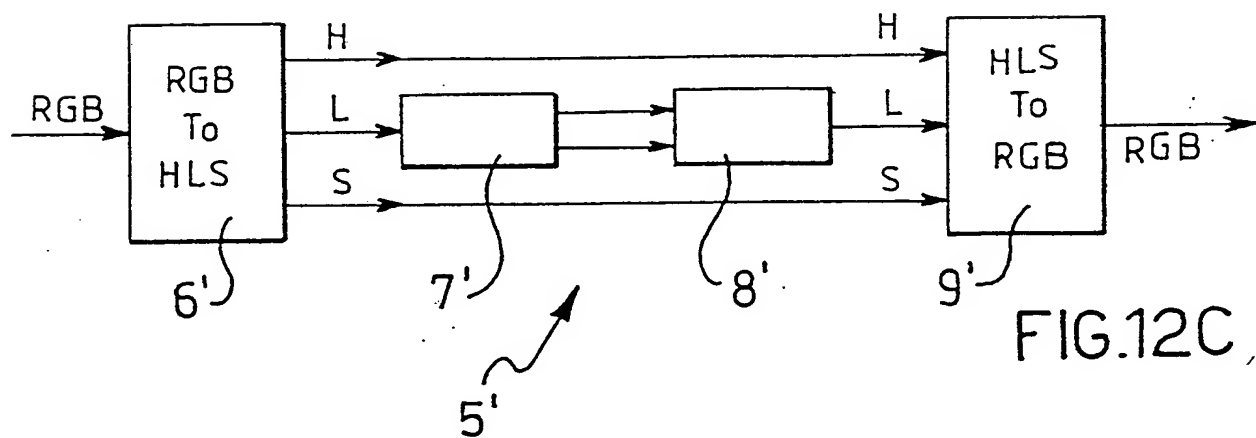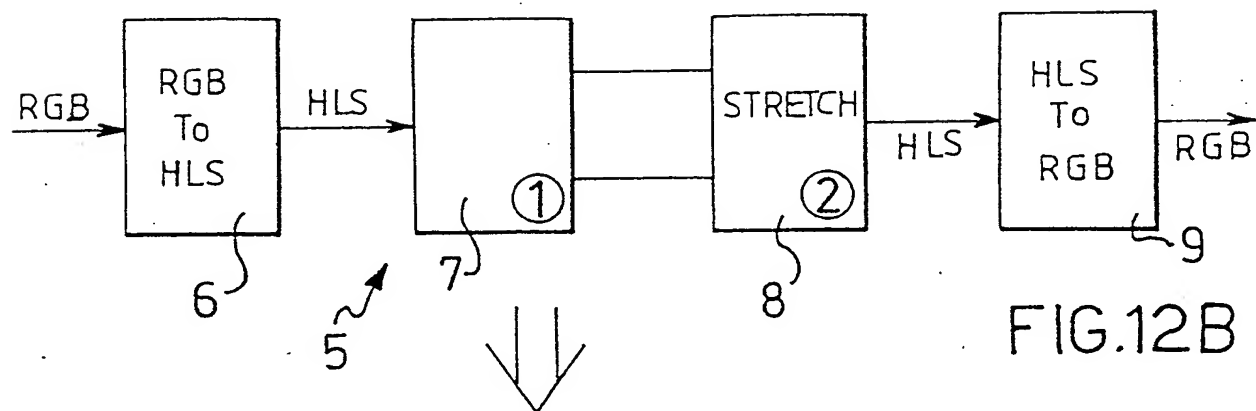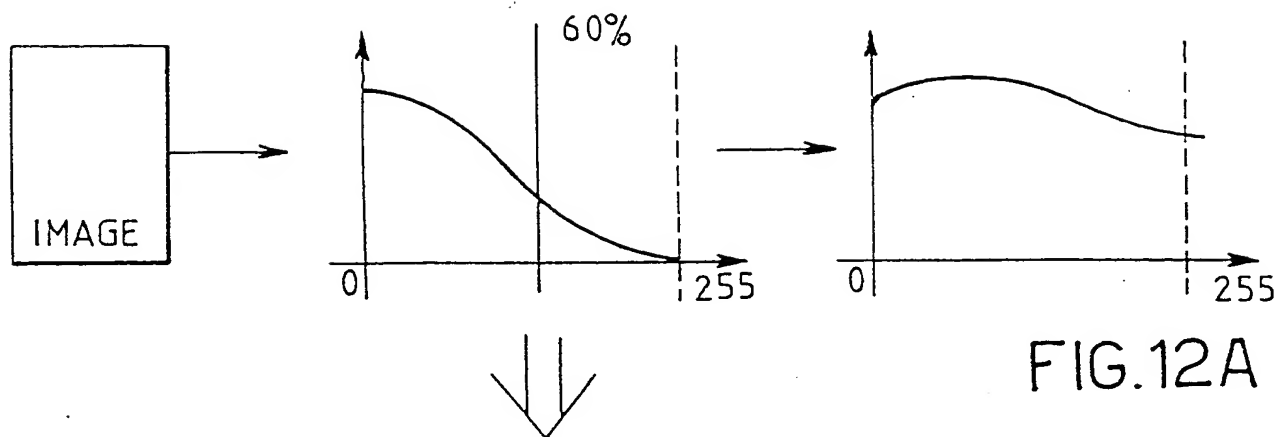

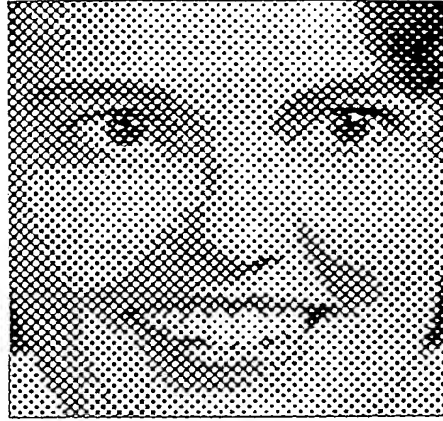


FIG. 13A


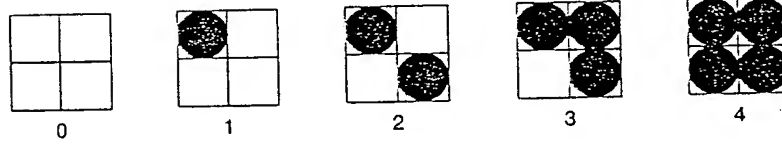


FIG. 13B



FIG. 13C

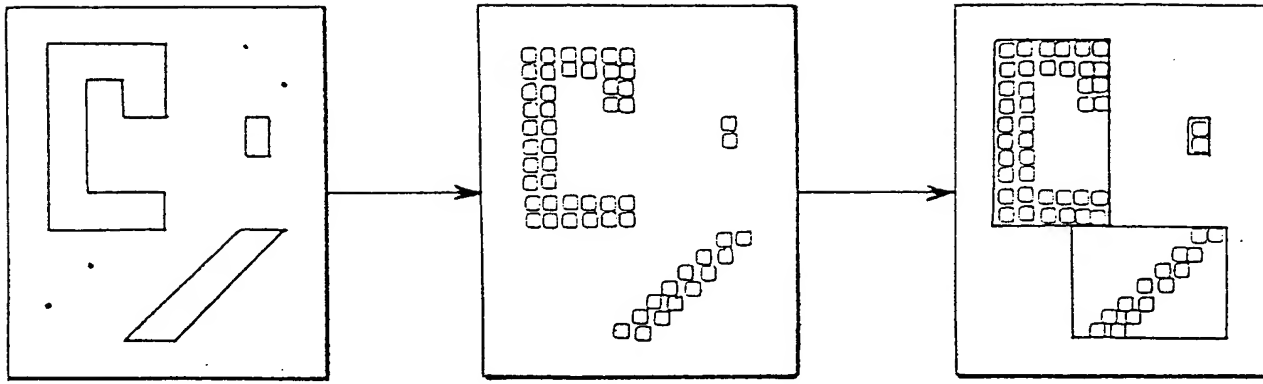


FORMAT 1

FORMAT 2


FORMAT 3

FIG. 14A


OR

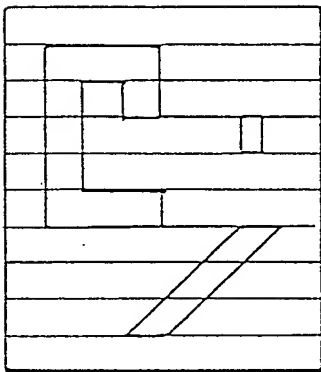

FORMAT 1

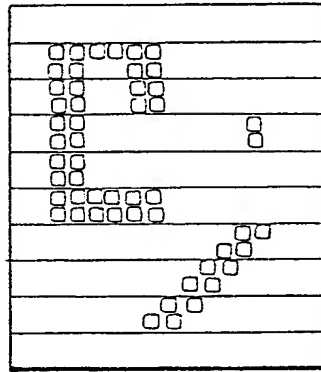

FORMAT 2

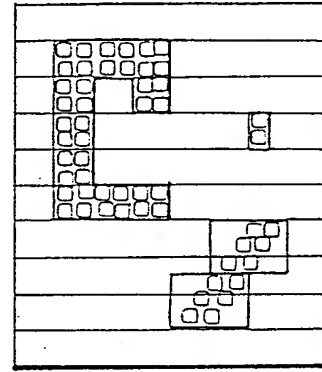

FORMAT 3

FIG. 14B

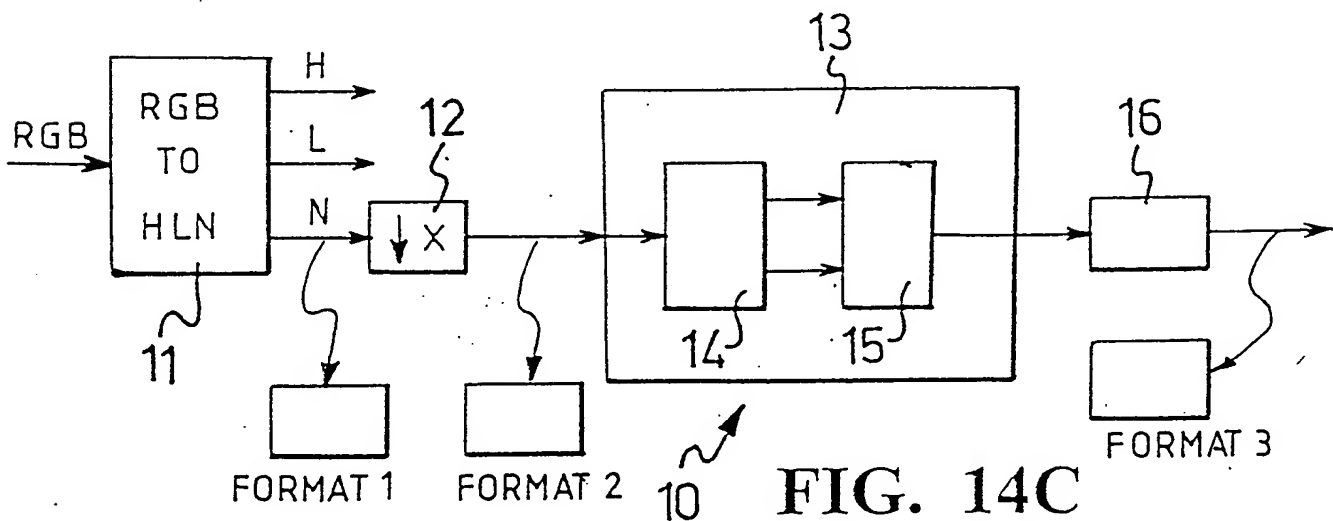


FIG. 14C

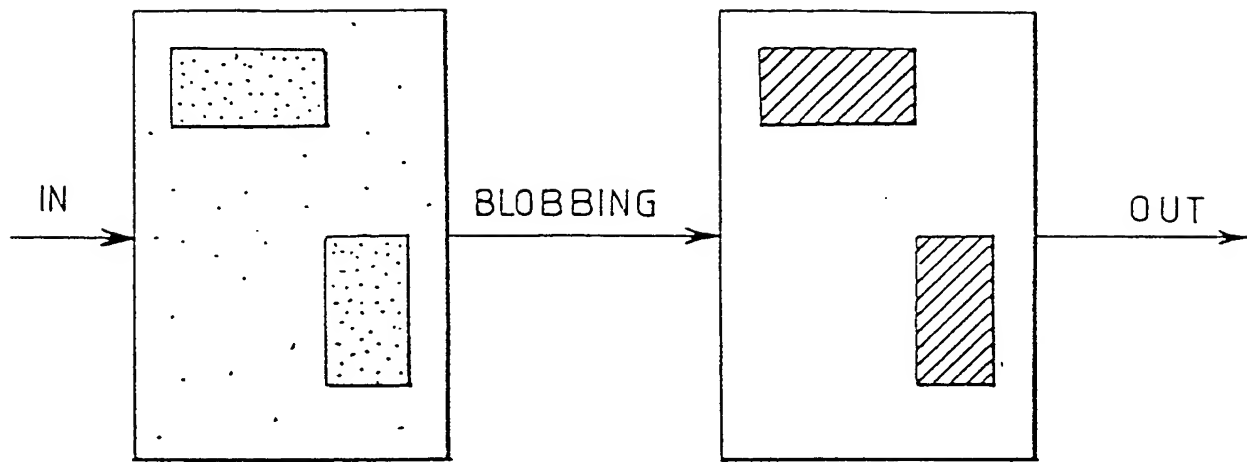


FIG. 16

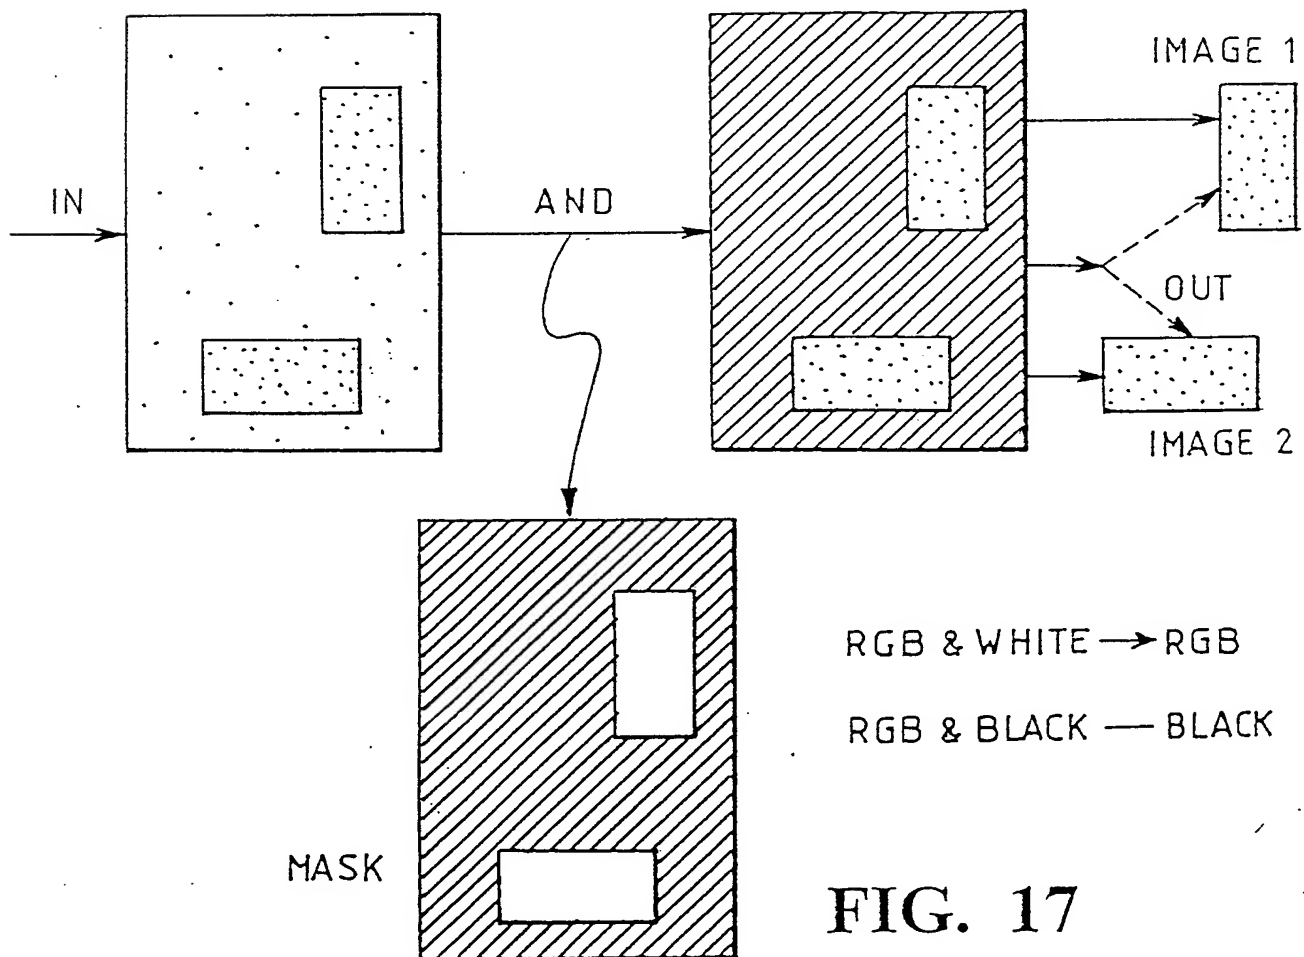


FIG. 17

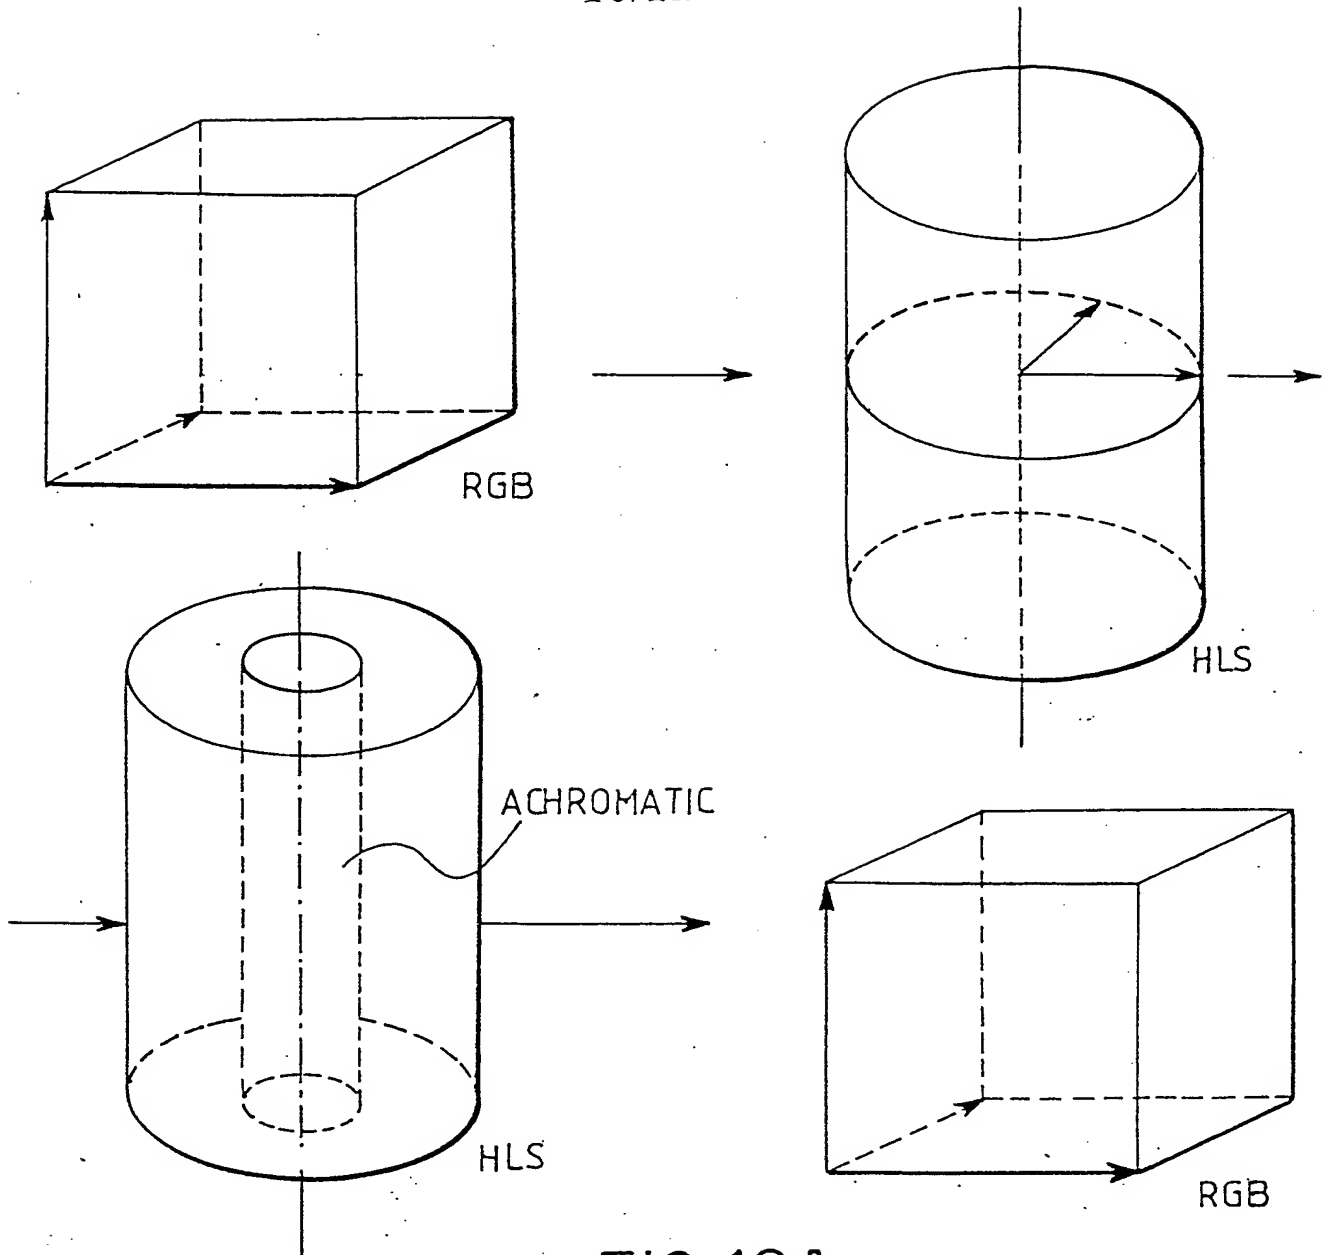


FIG.18A

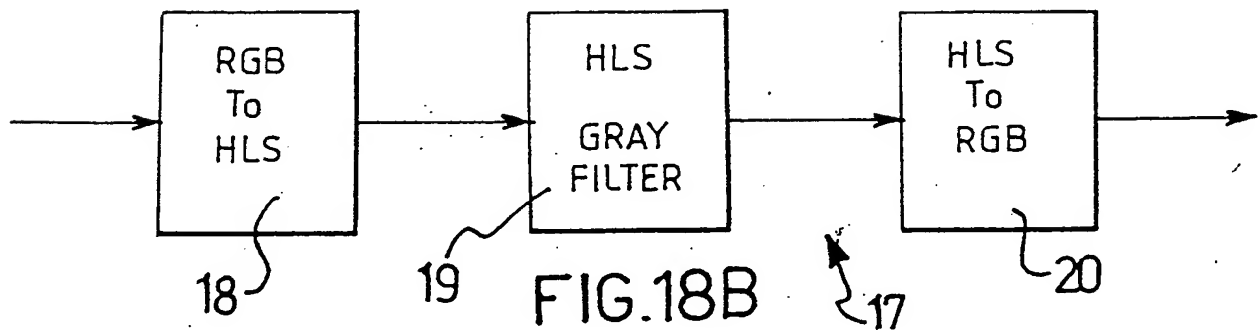


FIG.18B

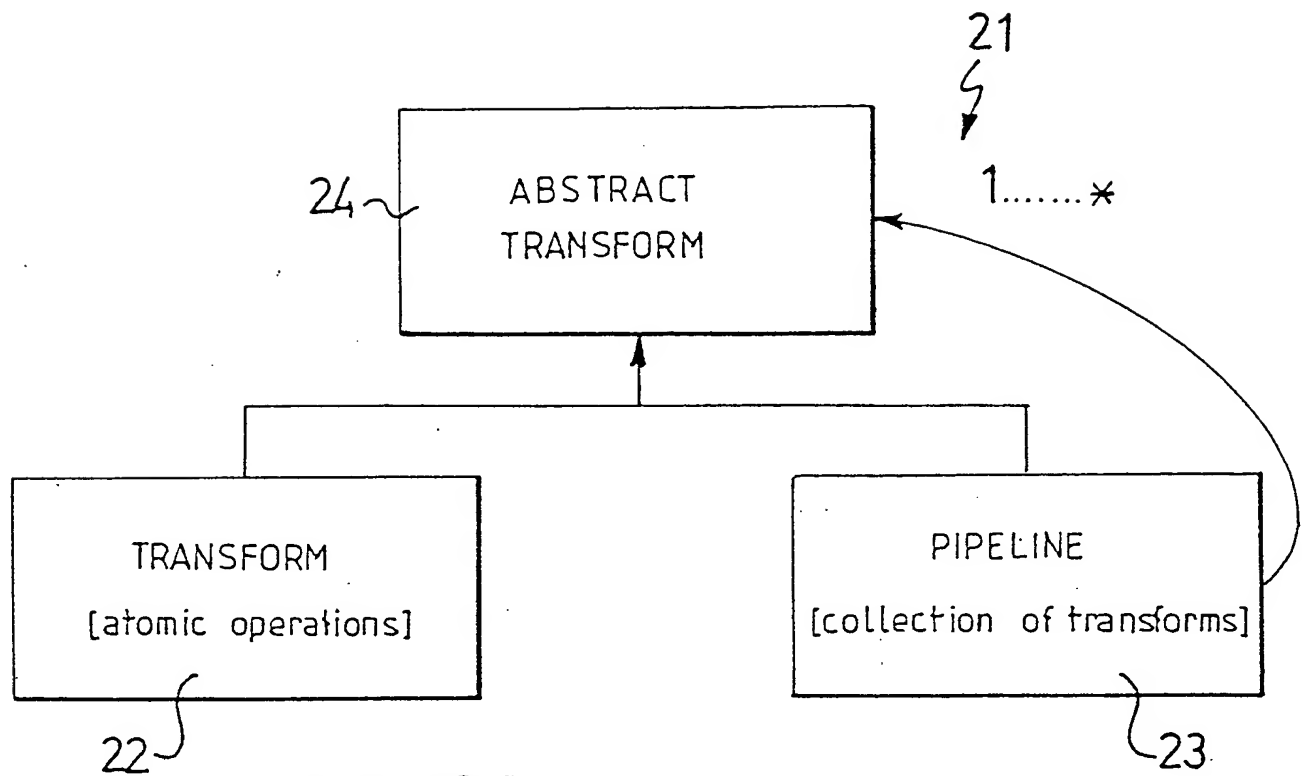


FIG. 19A

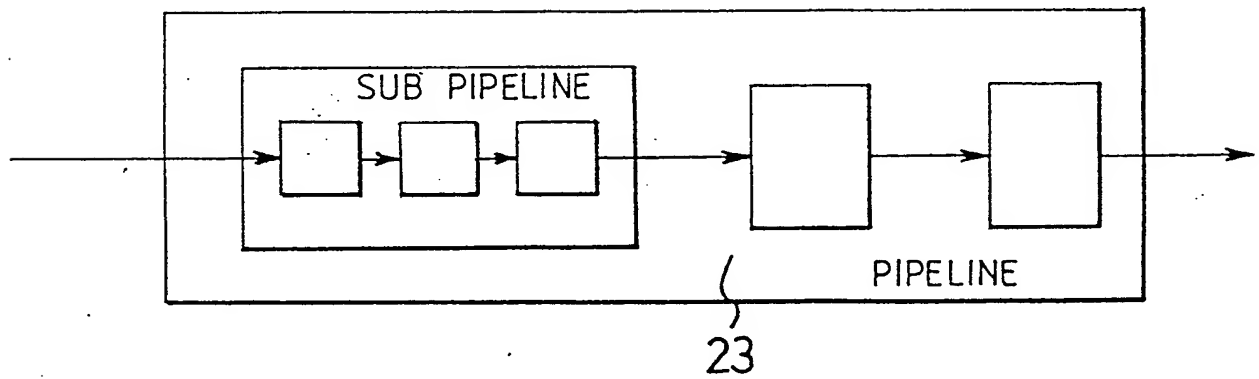


FIG. 19B

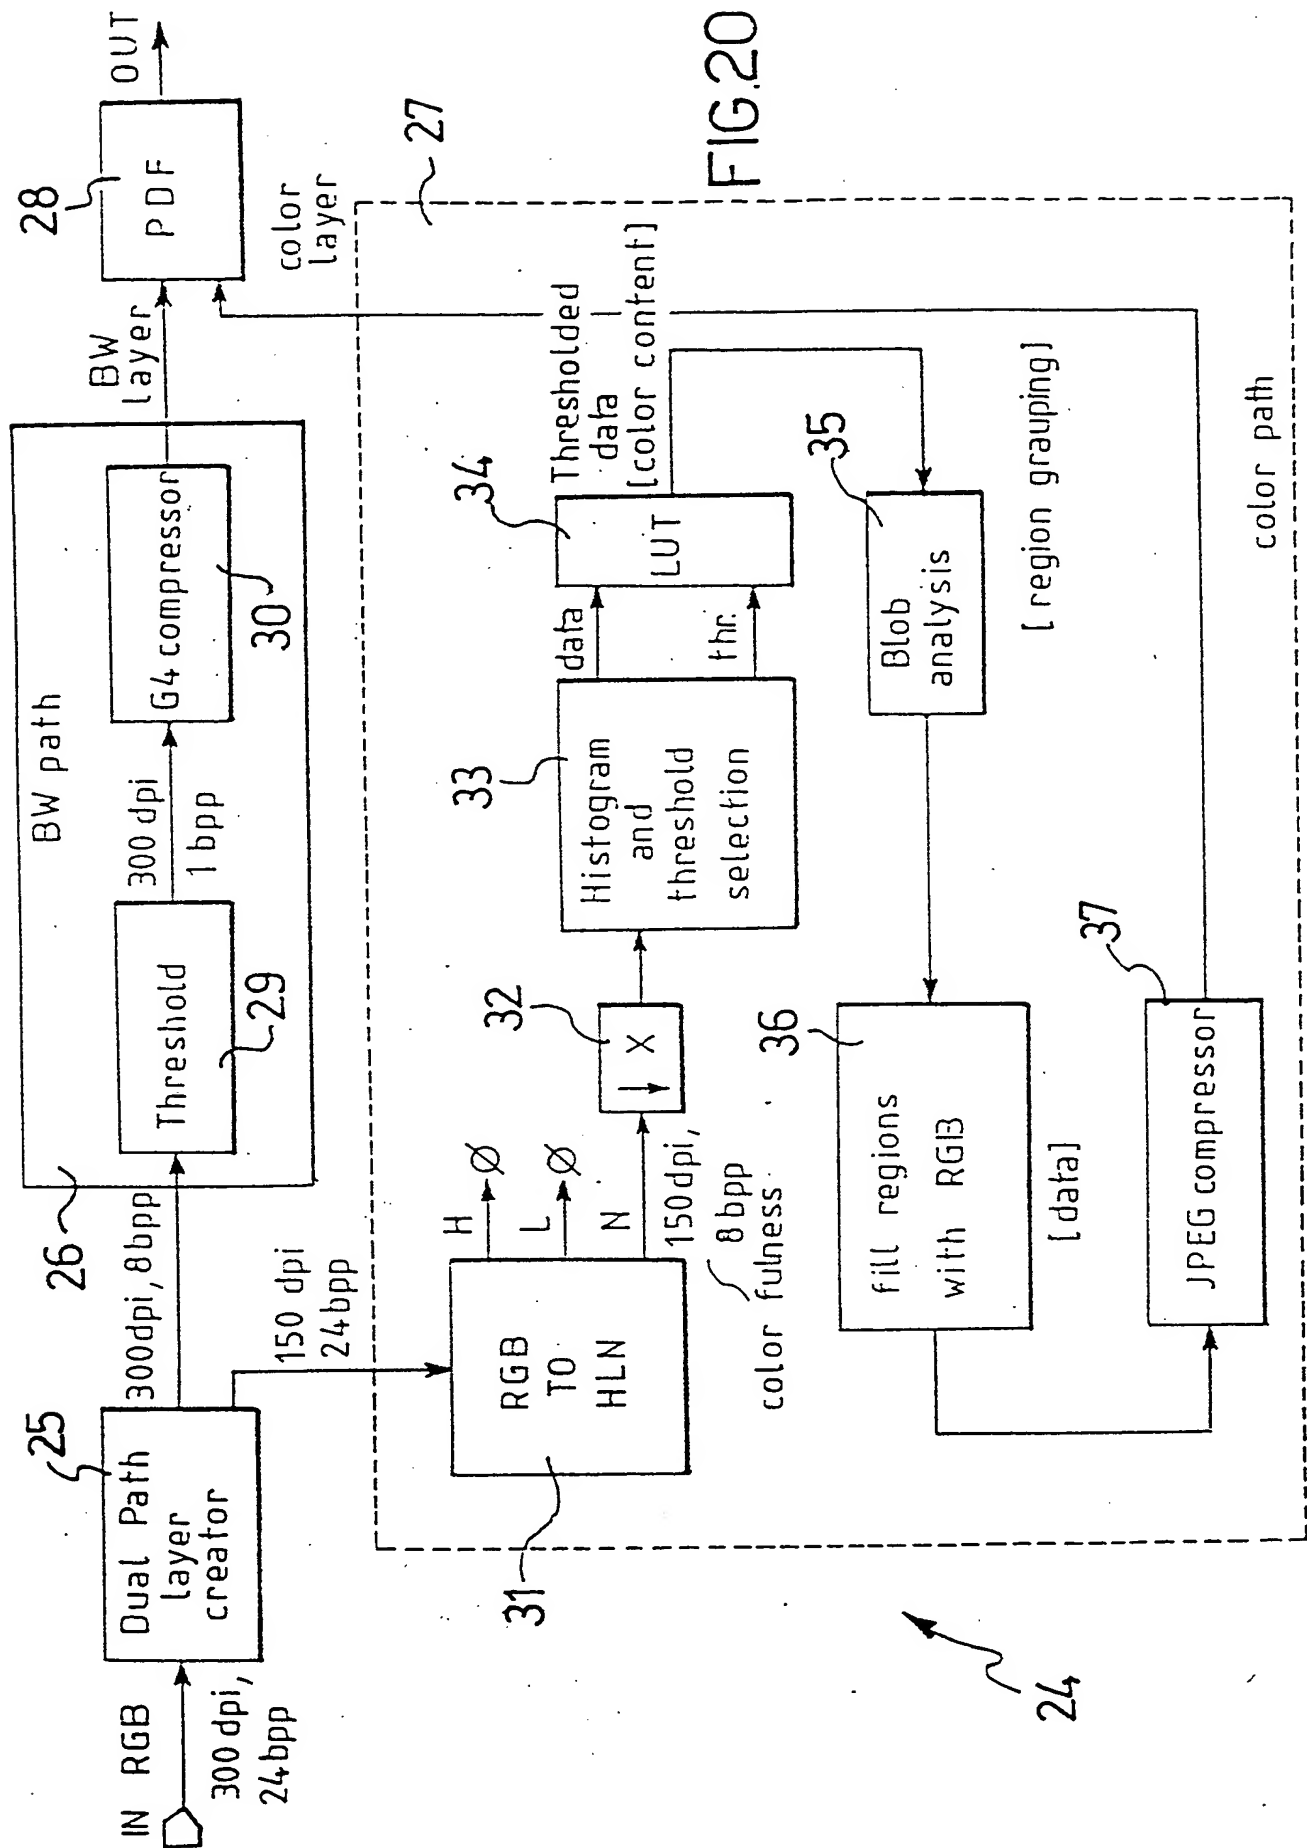


FIG. 20